

OPTIMA²CM

USER MANUAL



DIVE RITE®



This is the user manual for the Dive Rite O2ptima CM eCCR rebreather.

This user manual is proprietary and copyright Lamartek, Inc. 2020. It may not be reproduced, changed, or distributed without authorization from Lamartek, Inc.

All information contained in this manual has been carefully reviewed and is believed to be accurate, however it is subject to change. Rebreather technology is constantly and rapidly evolving. Please check www.diverite.com to ensure that you have the latest version of this manual.

Companies and/or product names cited in the manual are trademarks belonging to their respective companies.

The O2ptima CM is manufactured in the USA by:

Lamartek, inc. dba Dive Rite

175 NW Washington Street

Lake City, FL, 32055 USA

Phone (386) 752-1087

www.diverite.com



General Safety Statements and Warnings



- **DO NOT** use the O2ptima CM without successfully completing an O2ptima CM specific training program. Training on previous versions of the back-mounted O2ptima is not sufficient for diving the O2ptima CM.
- **DO NOT** use the O2ptima CM without reading and understanding this manual in its entirety.
- Reading this user manual **DOES NOT** replace unit specific training. This manual does not provide directions for diving with closed circuit rebreather equipment. This manual is only intended to be a guide for the proper maintenance, setup, operation, and basic service of the O2ptima CM rebreather.
- As with any piece of equipment, this rebreather will eventually fail. Even careful maintenance, assembly, and testing will not prevent this from happening. It is possible that any part of this unit **may fail at any time**. Because of this, it is essential that a separate, independent bailout system be taken by the diver on every dive. The bailout system must be configured to allow safe termination of the dive and return to the surface in the event of a malfunction at any point during the dive.
- All components of the rebreather must be in good working order and be carefully maintained, assembled, and tested to reduce the risk of failure.
- Participation in rebreather diving can result in **serious injury or death**. These risks can be reduced, but never eliminated.
- Knowledge and training are the best tools for avoiding accidents.
- Rebreather diving is a physically as well as mentally demanding activity.
- If you do not have adequate training, equipment, physical conditioning, and proper mind-set, do not get in the water.
- As the diver, **YOU have the final responsibility** for your own actions and safety while using this rebreather.



Table of Contents

General Safety Statements and Warnings	3
Introduction	6
Design Philosophy	6
System Overview	7
The Breathing Loop	8
Component Features & Functions	9
Counterlungs.....	9
Breathing Hoses & Fittings.....	9
Dive/Surface Valve (DSV)	9
Automatic Diluent Addition Valve (ADV)/Manual Addition Valve (MAV)	10
Oxygen Manual Addition Valve (MAV)	10
Overpressure/Dump Valve (OPV)	10
Scrubber Canister.....	11
Scrubber End Cap & Water Trap.....	11
Electronics Head	12
Oxygen Sensors.....	12
Controller	13
Electronics/Battery Canisters.....	13
HUD.....	14
Regulator, Hoses, & Gauge	14
Cylinders & Valve	15
Micropore ExtendAir Cartridge Overview	16
Assembling the O2ptima CM	18
Importance of Checklists.....	18
Gas Analyzation.....	18
Installing the Water Trap Tubes.....	18
How to Install a Micropore ExtendAir Cartridge.....	19
How to Pack the Scrubber	20
Installing the Scrubber End Cap & Water Trap.....	23



Installing the Electronics Head.....	24
Installing the Scrubber Assembly.....	26
Mounting the Electronics/Battery Canisters	27
Installing the Loop Hoses.....	27
Installing the DSV.....	28
Installing the Oxygen Cylinder, Regulator and Hoses.....	29
Basic Operation & Use	32
Harness Attachment	32
Oxygen Sensor Calibration.....	32
DSV Operation	33
Breathing on the Loop	33
Electronic vs Manual Operation	34
Diluent Injection.....	35
Servicing, Maintenance, & Cleaning.....	35
Post Dive Procedures & Cleaning.....	35
Oxygen Sensor Care	36
Oxygen Sensor Replacement	38
Battery Replacement	40
Battery Recommendations	41
Storage	41
Annual Service	42
Recommended Care Products	42
Technical Specifications	42
Revisions & Changes in Documentation.....	44
Appendix I: Checklists	44
Assembly Guide Checklist	45
Survival Checklist	46
Pre-flight Checklist.....	47
Post Dive Checklist.....	48
Appendix II: Galvanic Oxygen Sensors Applied to Closed Circuit Rebreathers	49



Introduction

Congratulations on your purchase of the O2ptima CM rebreather! First produced in late 2005, the O2ptima has been a leader in the rebreather market for over a decade. During that time it has been used for cutting edge exploration and world class expeditions all over the planet. Dive Rite has made a strong commitment to ensuring that it is one of the most reliable, capable, and high performing rebreathers on the market. The O2ptima design continues to evolve as refinements are made and new technology becomes available. The O2ptima CM represents the next generation of O2ptima design. The chest mounted configuration provides the advanced diver with new and unique opportunities for diving exploration. We are certain that this unit will provide you with many unforgettable hours exploring your underwater world.

Design Philosophy

The design parameters for the O2ptima were simple:

- Keep the breathing loop as short as possible
- Use proven, state of the art electronics
- Be fully compatible with the Micropore ExtendAir cartridge
- Maintain a rugged and durable package in the smallest profile possible

These parameters were originally chosen in order to produce a rebreather ideally suited to underwater cave exploration. The unique challenges of the cave environment demanded a unit that was as safe and reliable as possible while maintaining a minimal profile. The end result was a rebreather that is not only highly suitable for cave diving, but also any other type of technical diving where a direct ascent to the surface is not always possible.

By utilizing a horizontally mounted scrubber canister, the breathing loop was kept as short as possible. This helps to create the lowest possible work of breathing and allows the use of smaller diameter loop hoses. This in turn increases comfort and reduces diver fatigue. Internal water traps located in the counterlungs and canister end cap, combined with the use of the Micropore ExtendAir cartridge, greatly reduce the possibility of a “caustic cocktail.”

The O2ptima CM utilizes Shearwater electronics for their proven and unparalleled reliability and functionality.

At Dive Rite, we understand that one size does not fit all, so in addition to the standard O2ptima CM features there are a number of options to ensure a proper fit for any diver and mission. Contact Dive Rite or visit www.diverite.com for more details.



System Overview


The O2ptima CM is a chest mounted electronically controlled, constant PPO₂, fully closed circuit rebreather (eCCR). It has built-in decompression calculation and mixed gas capabilities. The following features come standard on the unit:

- Chest mounted counterlungs with 6 Liter total loop volume
- Redundant Shearwater DiveCAN electronics including heads-up display (HUD) and Petrel 2 controller (NERD controller optional)
- Dual use scrubber canister design that can be used with Micropore ExtendAir cartridges or packed with loose CO₂ absorbent
- Dive Rite DSV is standard
- Dual water traps in the counterlungs and scrubber lid
- Oxygen Regulator and hoses
- (4) AI or AST R22 Oxygen Sensors
- Sturdy outer cover utilizing abrasion resistant Rhinotek® fabric
- AL 13 oxygen cylinder with valve (optional)



The Breathing Loop

The O2ptima CM incorporates a chest mounted, dual counterlung design. The breathing loop consists of the DSV, breathing hoses and hose fittings, inhalation and exhalation counterlungs, scrubber canister, canister end cap, and electronics head. Gas flows from the diver—to the right counterlung—through the scrubber canister—to the left counterlung—back to the diver.

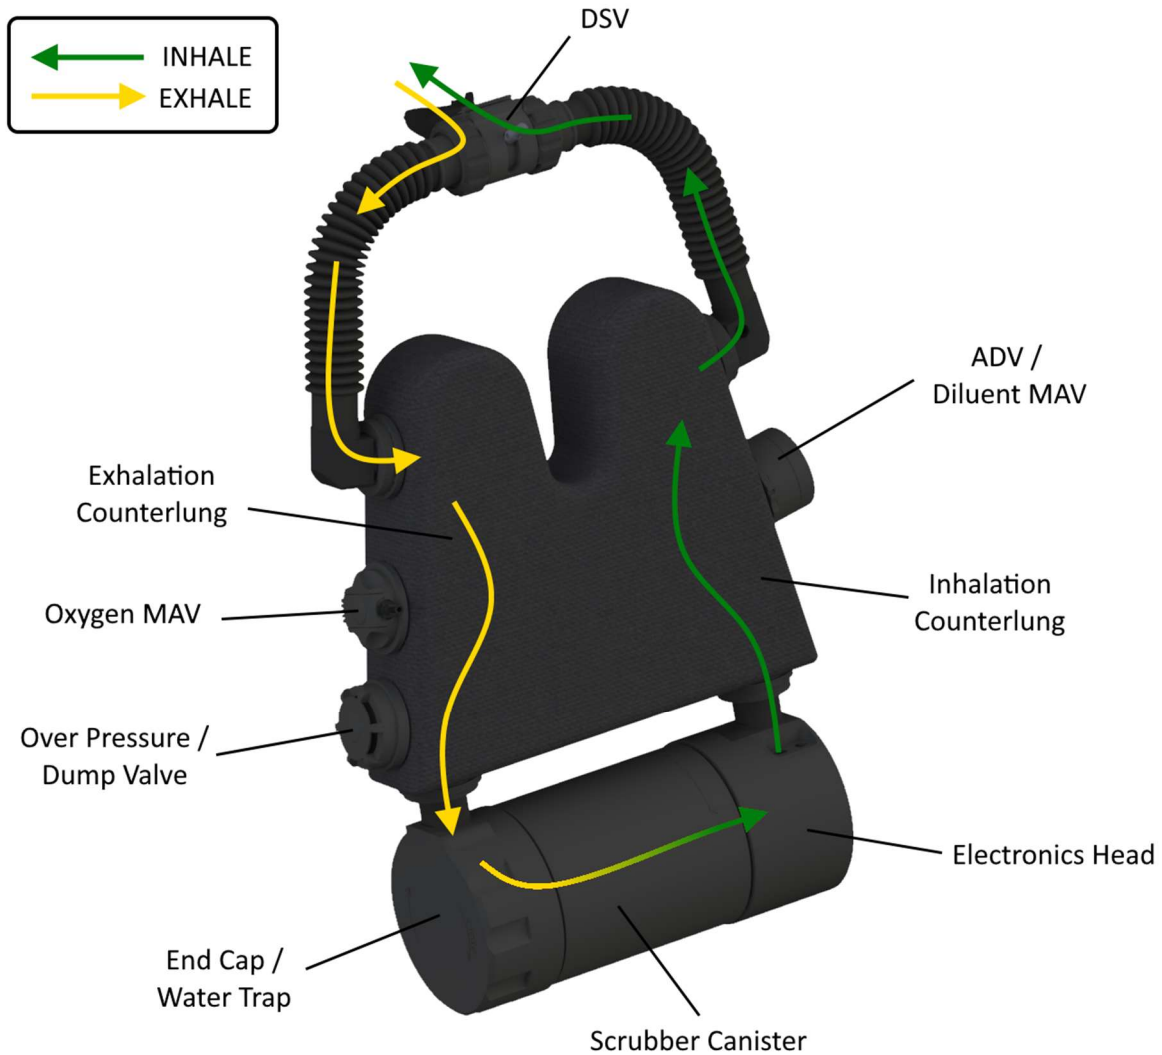



Component Features and Functions

Counterlungs

The O2ptima CM uses two integrated, chest mounted counterlungs. The counterlung position keeps them as close to the diver's lung centroid as possible providing excellent breathing characteristics in a variety of diver positions.

The counterlungs consist of an abrasion resistant outer bag and removable welded polyurethane inner bladders. The bladders are accessible through a zipper on the back side of the outer bag.

The bottom side of the counterlungs attach directly to the scrubber canister. The breathing loop hoses attach to the sides of the counterlungs using threaded connections.

The exhalation counterlung has an overpressure/dump valve located at the bottom of the lung. An internal water trap is located in the bottom of the exhalation counterlung to make de-watering the loop easy.



Breathing Hoses & Fittings

The hose diameter and lengths have been specifically chosen to provide the best balance of comfort and low work of breathing. The hose lengths are some of the shortest in the industry. This not only keeps the work of breathing low, but also reduces drag and uncomfortable vibrations occasionally encountered with excessive hose lengths when scooting or swimming against strong flow.

The hoses have threaded fittings attached to the counterlung ends. Each fitting utilizes a double O-ring seal to help ensure loop integrity. The hoses are 12 inches in length standard. Other sizes are available for improved fit on smaller divers.



Dive/Surface Valve (DSV)

The DSV has been completely redesigned from the ground up for exceptionally low work of breathing in the most compact design possible. Two high performance mushroom valves are used to ensure proper one way gas travel.

The lever on the front of the DSV is used to open the DSV for diving and close the DSV on the surface or during a bailout procedure to prevent water from entering the loop. The DSV utilizes a friction seal between the outer body and the inner barrel so there are no O-rings to wear out or replace on the barrel.





The DSV uses a bayonet style quick lock system to attach the hoses. To remove, simply press in the spring loaded white locking button and turn the connector ring 1/8 turn counterclockwise. The hose can then be pulled free. This feature allows fast and easy inspection of the mushroom valves and cleaning and maintenance.

Automatic Diluent Addition Valve (ADV) / Manual Addition Valve (MAV)

The ADV/MAV is mounted to the side of the inhalation counterlung. It utilizes a built in demand valve that is activated by negative loop pressure against a diaphragm in the same manner as a standard second stage regulator. It can also be manually activated by pressing directly on the diaphragm.



The ADV's position allows it to feed diluent gas directly to the DSV. This provides a fast, hands-free method of receiving a known breathable gas as well as supplying additional gas to increase loop volume.

The ADV/MAV comes with a standard LP inflator hose fitting to allow the use of any off-board diluent gas supply. For dives exceeding 130ft/40m, Dive Rite recommends upgrading this fitting to a high flow quick disconnect QC-6 fitting. Contact Dive Rite for details.

An inline shutoff is included to disable the ADV, however be aware that this also disables the MAV. The shutoff should also be used if the diluent gas supply is disconnected underwater to prevent water from entering the ADV/MAV.

The base of the ADV/MAV is screwed into a welded flange on the counterlung inner bladder.

Oxygen Manual Addition Valve (MAV)

The oxygen manual addition valve is a dry-suit style, side push valve. It uses a standard LP inflator hose connector. The valve allows the manual addition of oxygen and also permits the use of on-board as well as off-board gas supplies.

The oxygen manual add valve is located on the exhalation (right) counterlung. The valve is screwed into a welded flange on the counterlung inner bladder.



Overpressure/Dump Valve (OPV)

The O2ptima CM uses a special loop overpressure valve (OPV) located on the exhalation (right) counterlung. A specific spring is used to optimize the cracking pressure for rebreather counterlung use. Do not replace with a standard drysuit exhaust valve as they can have a much higher cracking pressure which can lead to lung overexpansion injuries.



This valve will normally be operated in the open position (turned fully counter-clockwise). Divers with a large tidal volume may find that they need to close the OPV slightly in order to maintain proper loop volume. The valve can also be manually opened by pressing on the valve. The valve is screwed into a welded flange on the counterlung inner bladder.



During an ascent, the gas in the loop will expand, increasing buoyancy and slightly increasing the breathing effort. Even though the maximum volume in the O2ptima CM's breathing loop is relatively small, it is important to set the OPV properly so that buoyancy shifts will be kept to a minimum without any diver action.

The OPV is also used for de-watering the loop. This procedure will be covered in your O2ptima CM class.

Scrubber Canister

The scrubber canister contains the scrubbing media that removes CO₂ from the breathing loop. The O2ptima CM uses an axial style scrubber canister and can be used with either Micropore ExtendAir cartridges or loose packable CO₂ absorbent.



Assembly is slightly different depending on which scrubber media is used. The wave spring and top plate with screen are not used when using an Extendair cartridge. The finger nut is reversible. It is used in one direction when packing loose CO₂ absorbent and is flipped over when using Extendair cartridges. See the **How to Pack the Scrubber** section for more information on properly setting up the scrubber canister.

Scrubber End Cap & Water Trap

The scrubber end cap contains a snap-in water trap in the shape of a cone. This shape prevents excess water from entering the scrubber canister regardless of the diver's position in the water.



The shape of the cone also assists in mixing the exhaled gas with added oxygen into a homogenous blend. The result is even gas flow through the scrubber canister and accurate readings by the oxygen sensors.

The end cap has an O-ring and a flat seal that seals against the scrubber canister and an additional O-ring that seals the water trap. These O-rings and seal require cleaning and maintenance and should be replaced on an annual schedule at a minimum.

The end cap attaches to the scrubber body by aligning the marks on the cap and body, pressing the cap into place, and the turning the cap clockwise until the mark is aligned with the "locked" position marking.



Electronics Head

The electronics head contains the solenoid, oxygen sensors (4), sensor disk, sensor wiring harness, and oxygen injection premix tube. These components are responsible for analyzing the oxygen content of the breathing gas and injecting oxygen as needed.

The controller (Shearwater DiveCan system) interprets the readings from the oxygen sensors and makes decisions on when to add oxygen via the solenoid.

The injected oxygen travels through the premix tube to the exhalation side of the scrubber canister where it is blended with the loop gas before going through the scrubber material. This reduces O₂ “spikes” by ensuring that the gas mixture is homogenous before passing over the oxygen sensors.



Oxygen Sensors

The O2ptima CM uses four oxygen sensors. These sensors are threaded into the sensor disk mounted inside the electronics head. Dive Rite uses both Analytical Industries, Inc. and American Sensor Technologies, Inc. type R22D sensors.

Oxygen sensors have a finite life. They are a consumable item and must be replaced at regular intervals. They are typically replaced during the annual service, but may need to be replaced prior to this.

The sensor labeling includes a “Sell by” date of 4 months after manufacture and a “Do not use after” date of 16 months after manufacture. Sensors must not be used after this date even if they appear to still be functioning correctly.

Four sensors are used to provide redundancy and the ability to cross check their values against each other to determine if a sensor is not reading correctly. Sensors 1 and 2 are shared between the controller and the HUD. Sensor 3C is only connected to the controller, and sensor 3H is only connected to the HUD. By comparing sensor readings between the HUD and the controller it is easy to determine if a sensor is not reading correctly.

If sensor values 1, 2, and 3C do not agree, the controller automatically uses a voting logic to make an educated guess of which sensor is not reading correctly. Having an independent “4th sensor” display on the HUD allows the diver to independently verify the controller’s voting logic.

For more information on oxygen sensors, see the **Oxygen Sensor Care** section and also **Appendix II: Galvanic Oxygen Sensors Applied to Closed Circuit Rebreathers** by Analytical Industries, Inc.





Controller

Dive Rite has chosen to use Shearwater electronics to control and monitor the O2ptima CM. The controller is a DiveCAN Petrel 2 handset. The controller allows diver control of the PPO2 setpoint and PPO2 monitoring of oxygen sensors 1, 2, and 3C. It also functions as a full featured dive computer displaying depth, dive time, decompression information, and other important dive information.

It is recommended to use a second standalone dive computer with decompression information as a backup in addition to the controller.



For detailed information on the DiveCAN Petrel controller, please see the **Shearwater Petrel DiveCAN Rebreather Controller Model Operations Manual**.

Dive Rite now offers an optional Shearwater NERD controller for the O2ptima CM which allows full set-point control without a Petrel 2 controller. Contact Dive Rite for more information.

Electronics/Battery Canisters

There are two external electronics & battery canisters on the O2ptima CM. They are mounted between the scrubber canister and the counterlungs in elastic sleeves on the bottom of the outer bag.

One canister contains the SOLO (SOlenoid and Oxygen) electronics board and battery. The battery is a standard 9 volt battery that powers the SOLO board as well as the oxygen solenoid. The Petrel 2 controller handset has its own internal battery and does not rely on the 9 volt battery.

The other canister contains the OBOE (Oxygen BOard Electronics) board and battery. The OBOE board controls the HUD. The battery is a standard AA type. This battery only powers the OBOE board and HUD.

By locating the batteries in these external compartments, they are completely isolated from the head and the breathing loop. This is important because as batteries age or are damaged they can release toxic chemicals. Obviously this is not something you want to have in your breathing gas.

The batteries are accessed via a threaded cap on the end of each canister. The caps are double O-ring sealed to ensure water integrity. These O-rings must be inspected and maintained when the canisters are opened to reduce the chance of flooding. See the **Battery Replacement** section for additional information.

The electronics canisters connect to the controller and HUD using wet pluggable, waterproof connectors. Regular lubrication of the inside of these connectors with a light coating of silicone grease such as Molykote 111 will increase their usable life.





HUD

The O2ptima CM includes a Shearwater HUD (Heads-Up Display). The HUD displays the PPO2 readings of oxygen sensors 1, 2, and 3H. These values are displayed using three columns of LEDs. Each column represents a different sensor. The colored LEDs flash using a modified Smither's code to convey the PPO2 values. A "color blind" mode is also available. The HUD can be setup for right or left eye operation. The HUD can be turned on manually by pressing the button on the end of the housing. There are also wet contacts which automatically turn the unit on in case it was not turned on prior to the dive.



Your life depends on always knowing the PPO2 in the breathing loop while diving a rebreather. Do not make assumptions about how the HUD displays PPO2 values. Previous versions of the HUD used different blink patterns. Refer to the latest **Shearwater HUD User Manual** for a detailed description of the HUD blink pattern and operation.

The Shearwater NERD (Near Eye Remote Display) is also available as an option. (<https://www.shearwater.com/products/nerd/>) The NERD replaces the standard HUD providing a numerical readout of the 3 sensor PPO2 values and also serving as a backup computer with fully redundant decompression and dive information. Dive Rite now offers a controller version of the NERD which allows full set-point control without using a separate Petrel 2 controller. Contact Dive Rite for more information.

Regulator, Hoses, & Gauge

A Dive Rite first stage with DIN connector and hose assembly is included for the oxygen supply. First stage intermediate pressure (IP) is set to 85 psi for the oxygen regulator. The oxygen regulator IP must be set no higher than 85psi due to the maximum rated pressure of the solenoid.

A diluent regulator and hoses are not supplied with the O2ptima CM. The unit is only intended to be used with an off-board diluent supply and it is up to the diver to supply these components as there are a wide variety of possible configurations.

An over-pressurization valve (OPV) is installed in the oxygen first stage for safety. Because there are no second stages installed there is no other way for excess pressure to be released. The over-pressurization valve must be in place in the event of a first stage high pressure seat failure to prevent high pressure gas from reaching all of the downstream components.

An OPV that is releasing pressure indicates a malfunction and the dive should be terminated immediately. The OPV should be inspected for bubbling during the S-drill at the beginning of the dive.

The first stage needs to be serviced annually by an Authorized Dive Rite service center or directly by Dive Rite. Call Dive Rite directly (1-800-495-1046) or email support@diverite.com to schedule service.





Braided nylon Airflex LP hoses are used for oxygen gas supply on the O2ptima CM. Airflex hoses are flexible, yet tough. The hose lengths are optimized for streamlined routing.

A small button SPG is included to monitor oxygen tank pressures. A BAR gauge is used to help simplify gas consumption calculations.

An inline shutoff with safety lock is included. **This should be closed any time the oxygen supply hose is disconnected underwater to prevent water from entering the solenoid causing damage or failure to operate.** Once the oxygen supply hose is connected, turn the gas supply on and purge the line using the oxygen MAV before opening the inline shutoff. Once the shutoff is open, install the included safety lock clip to prevent accidental oxygen shutoff.

Cylinder & Valve

The base O2ptima CM does not include an oxygen cylinder, however they are available. Dive Rite recommends an aluminum 13 cf (2L) cylinder for on-board oxygen use. The diver may also choose to sling an oxygen bottle of their choosing separately for off-board use.

The on-board cylinder is held in place with two included adjustable cam straps. No additional cylinder mounting hardware is necessary.

The AL13 cylinder is a good compromise between weight and gas volume. It is an excellent choice for general rebreather diving. Other recommended cylinders that will work as on-board bottles with the O2ptima CM are:

- Aluminum 20 cf (3L)
- Steel AA LP13 cf (2L)
- Steel AA LP15 cf (2L)
- Steel AA LP27 cf (4L)
- Steel AA HP32 cf (4L)

However, the larger cylinders may have undesirable buoyancy characteristics when used as on board cylinders. Divers should select cylinders based on their dive duration, travel logistics, and buoyancy characteristics.






Micropore ExtendAir Cartridge Overview

(Information from www.microporeinc.com)

ExtendAir® adsorbent technology is a combination of a microporous gas adsorbent sheet and the geometry in which it is utilized. The adsorbent material is manufactured with a proprietary process into a microporous sheet that can be made into different thicknesses and widths, using the same chemistry as in granular adsorbents.



Sheets of adsorbent material are wrapped around a core to form an

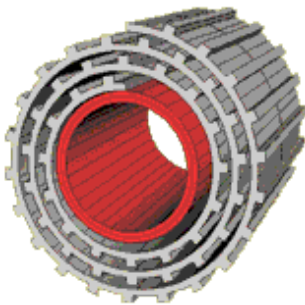

ExtendAir® cartridge. The molded ribs in the material create channels through which the breathing gases flow. One of the unique features of an ExtendAir® cartridge is that the breathing resistance of the adsorbent can be precisely controlled by varying rib height and spacing. This controlled channeling of the breathing gases results in a very uniform reaction zone within the adsorbent.

In a granular canister, gases seek the path of least resistance through the bed. The flow pattern can be very random and will certainly vary from person to person. Learning to load a granular canister requires instruction to learn the proper technique. Optimal loading of the canister requires tapping to achieve a uniform bed of granules. This takes time and can cause dusting of the adsorbent. All of this leads to variations in duration, wasted adsorbent and the potential for "caustic cocktail".

In contrast to a granular system, ExtendAir® cartridges use channels, molded in at the factory, that remain constant and controlled by the manufacturing



process. The user simply places the cartridge into the canister, without any need for tapping or shaking as the canister is being loaded. As such, the duration variability due to irregular granule settling patterns, as well as variability due to individual loading technique are completely eliminated. Eliminating this variability will directly translate into longer minimum duration, and a +/-5% variation in duration at any test condition (granules can vary up to +/-30%).




An important concept to understand with ExtendAir® cartridge technology is that the gas flow distribution through the cartridge must be uniform in order for the system to perform optimally. For example, one way to visualize flow through an ExtendAir® cartridge system is to take a bunch of soda straws in your hand (50 or so). What would happen if you blew air down through just a group of 5 straws? All of the air would flow down those five straws, and none of the air would flow through the other 45. The same thing would happen if you blew air into just one side of an ExtendAir® cartridge canister: all of the air would flow through that side only.



The end result of this uniform flow is full utilization of the adsorbent in the cartridge.

To achieve full adsorbent utilization, Micropore designs canisters to achieve a +/- 5% flow distribution at the inlet face of the ExtendAir® cartridge. This is accomplished through various engineering techniques such as diffusion screens and flow testing of the breathing loop. The result is a system engineered to perform consistently independent of individual loading techniques.

The combination of Micropore's ExtendAir® adsorbent manufacturing process, along with the parallel flow cartridge design, turns out to be extremely efficient. Installing an ExtendAir® Cartridge (EAC) is relatively simple, and takes seconds to perform. The O2 injection tube runs through the center of the EAC and with the use of a plug any possibility of "CO2 Channeling" is prevented.

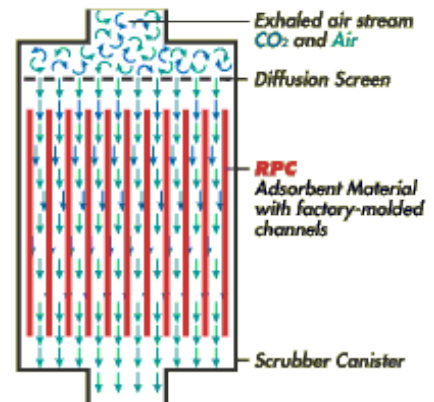



Assembling the O2ptima CM

This section will explain basic assembly procedures of the O2ptima CM. These instructions will serve as a guideline for correct initial assembly as well as disassembly necessary for transportation or maintenance.

Importance of Checklists

Many rebreather accidents and fatalities could have been prevented with the use of assembly and pre-dive checklists. There is nothing particularly difficult about assembling a rebreather, however there are many small yet important steps in the process. A small oversight such as forgetting to re-install an O-ring can have disastrous consequences.

We are all human and as such are susceptible to distraction and lapses in memory. There is overwhelming evidence pointing to the efficacy of checklists in preventing errors in complex technical procedures. It is highly recommended that you use a written or digital checklist for both assembly and pre-dive checks before every dive. See the **Checklists** section in this manual for assembly and pre-dive checklists.

Gas Analyzation

The most important rule of rebreather diving is to always know what gas is in the breathing loop. This process begins with analyzing the contents of your cylinders.

Sensor calibration is performed assuming a certain percentage of oxygen, however the only way to know what percentage of oxygen the cylinder actually contains is to analyze it. If the actual percentage of oxygen in the cylinder is different than what is assumed, it could lead to an incorrect calibration resulting in a different gas mix in the loop than what is displayed on the HUD and controller. This could result in oxygen toxicity or errors in decompression calculations.

It is highly recommended that both oxygen and diluent cylinders, along with any bailout cylinders, be analyzed and the contents labeled on the cylinder prior to assembling the unit. .

Installing the Water Trap Tubes

Begin by installing the water trap tubes into the counterlungs. Lay the outerbag with the back side facing up. One end of each tube is slightly flared to prevent it from sliding too far into the fitting. Note that the tubes are different and one is labeled "IN" for "Inhale" and one is labeled "EX" for "Exhale". The Inhale tube has holes toward the bottom to allow water to drain from the inhale loop back through the scrubber. The Exhale tube has holes at the top to allow for water trapping while ensuring the counterlung bladder cannot block off the end of the tube causing hard breathing.

Inserting the non-flared end first, slide the correct tube into each counterlung from the bottom fitting until it is fully inserted (See **Figure 1**). Note that the exhale side tube will have more resistance when inserting because there is an O-ring inside of the exhalation counterlung fitting but not the inhalation side fitting. This is to trap any water inside the exhalation counterlung for de-watering through the OPV. The O-ring is not needed on the inhalation side.



Figure 1 – Inserting Water Trap Tubes—Inhale on Left, Exhale on Right (note hole location)

How to Install a Micropore ExtendAir Cartridge

The next step in the build process is to assemble and install the CO₂ scrubber canister. The O₂pitma can be used with either the Micropore ExtendAir cartridge or it can be packed with loose granular CO₂ absorbent. This section will deal with using the ExtendAir cartridge. If you are using loose granular absorbent, skip to the next section, **How to Pack the Scrubber**.

To use an ExtendAir cartridge, begin by inspecting all of the scrubber components. Look for any damage, dirt, debris, or excess lubrication on the scrubber canister, ExtendAir cartridge, scrubber end cap, electronics head, bore plug nut, and seals and O-rings. Any damage or contamination can cause a loss of water integrity and flooding of the breathing loop.

Next, remove the ExtendAir cartridge from its packaging and, using a permanent marker, mark the installation direction on the side and/or end of the cartridge. If the cartridge is removed between dives and then later reinstalled, it is critical that the cartridge be reinstalled in the same orientation to prevent premature CO₂ breakthrough. Install the cartridge by sliding it all the way into the canister (See **Figure 2**).



Figure 2 – Installing ExtendAir Cartridge



Next, install the bore plug nut with the tapered end toward the cartridge. This tapered end will seal against the center bore of the cartridge. Tighten by hand until snug (See **Figure 3**). The included wave spring and top plate with screen are not used when using an ExtendAir cartridge. The canister is now ready to be installed on the unit.



Figure 3 - Bore Plug Installation for EAC

How to Pack the Scrubber

The scrubber canister can be packed with approximately 5 pounds of loose granular CO₂ absorbent. Dive Rite recommends Intersorb 812 or Sofnolime 797 (8-12 mesh) granular absorbent. 408 (4-8 mesh) is not recommended. It is important to use fresh absorbent for every dive. Granular absorbent should never be reused.

To pack the scrubber, begin by inspecting all of the scrubber components. Look for any damage, dirt, debris, or excess lubrication on the scrubber canister, scrubber end cap, electronics head, bore plug nut, and seals and O-rings. Any damage or contamination can cause a loss of water integrity and flooding of the breathing loop.

Dive Rite includes a filter disc that should be used when packing the scrubber with granular absorbent. This is to reduce the amount of dust that reaches the head and the rest of the breathing loop. It is placed in the bottom of the scrubber body, underneath the stainless steel mesh screen. This filter is optional when using an ExtendAir cartridge. The filters are reusable but will need to be replaced eventually. Replacements can be ordered from Dive Rite in packs of 3.

Ensure that the filter is in place and the stainless steel screen mesh is correctly seated on top of it in the bottom of the scrubber canister (See **Figure 4**).



Figure 4 – Filter and Screen Installed in Scrubber Canister



Begin pouring granular absorbent into the canister (See **Figure 5**).



Figure 5 - Pouring Scrubber Media

Fill the canister approximately half full and then tap around the outside of the canister to settle and level the absorbent (See **Figure 6**).



Tap sides of canister
to settle absorbent

Figure 6 - Tap to Settle

Continue filling with absorbent until it is approximately $\frac{1}{4}$ inch (6mm) from the top of the canister. Again tap around the outside of the canister to continue settling and compacting the absorbent. If necessary, add more absorbent to bring the fill level back to $\frac{1}{4}$ " (6mm) from the top of the canister.

Place the top plate with attached screen on top of the canister with the screen side down. It should be flush with the inside edge of the canister (See **Figure 7**). If it is not, add or remove absorbent and relevel until it is. Note—the wire handle on the top plate is only for removing the plate. It is not a carry handle for the scrubber.



Figure 7 - Proper Fill Level

Next, place the wave spring around the stainless steel center tube, on top of the top plate. Finally, orient the nut with the tapered side up and thread it onto the center tube (*Note that the nut is installed in one direction when using an EAC and the other direction for a packed scrubber). Make sure that the spring sits in the small counterbore in the nut. This keeps the spring centered on the top plate (See **Figure 8**). Hand tighten the nut to compress the wave spring against the top plate. Do not overtighten the nut.

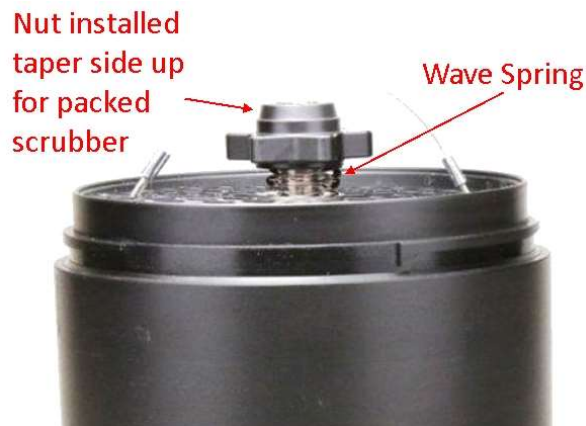


Figure 8 – Spring & Nut Orientation



Figure 9 - Nut Tightened

The nut and spring are not intended to apply pressure to “pack” the scrubber. They are only to ensure an even pressure is held on the top plate after properly packing it.

The canister is packed correctly if shaking the canister does not result in noise being heard from the absorbent. Any movement of the absorbent can lead to channeling and premature CO₂ breakthrough. If needed, remove the lid and continue tapping the sides of the canister and adding more material as necessary.

Clean up any excess absorbent dust before installing the scrubber canister. The dust will quickly react with any exposure to water and can create a caustic solution in the breathing loop.



Installing the Scrubber End Cap & Water Trap

The cone shaped water trap snaps into the end cap and can be removed for maintenance and cleaning. There is a large orange O-ring sealing the edge of the water trap (See **Figure 10**).



Figure 10 - Water Trap Sealing O-ring

Clean and lightly lubricate this O-ring with Tribolube 71 and then snap the water trap into place. Next, clean, lubricate and install the large sealing O-ring (See **Figure 11**).



Figure 11 - Installing Water Trap & Large Sealing O-ring

There is a large orange flat seal that is pressed into the water trap. It is recommended not to remove this seal unless replacement is necessary as it is difficult to reinstall.

If the flat seal must be removed, reinstall the clean and lightly lubricated seal by pressing into place on opposite sides and then slowly, working back and forth, flattening it into the groove (See **Figure 12**).



Figure 12 - Inserting Flat Seal



Figure 13 - Complete End Cap Assembly

Figure 13 shows the completed end cap assembly ready for installation.

To install the end cap, align the arrows on the end cap and body, push the head into position, and then rotate clockwise until the end cap arrow is aligned with the “LOCKED” position (See Figure 14).



Figure 14 - Locked Position

Installing the Electronics Head

Check that the orange electronics head O-rings and flat seal are clean and lubricated. Dive Rite recommends lubricating these seals with Tribolube 71 grease.

Confirm that the small orange O-ring is in place on the premix tube. The O-ring should be above the sensor disk. To ensure that it is in the right spot, lay your fingers on the disk and the O-ring should be above your fingers (See Figure 15). When the canister is installed it will push the O-ring down to seal against the stainless steel tube in the center of the canister.



Figure 105 – Premix Tube O-ring Position

Install the head by inserting the premix tube into the center tube of the body, aligning the arrows on the head and body (See **Figure 16**), pushing the head into position, and then rotating clockwise until the head arrow is aligned with the “LOCKED” position (See **Figure 17**).



Figure 11 – Installing Electronics Head

Figure 17 - Locked Position



Figure 128 – Complete Scrubber



Figure 18 shows the complete scrubber assembly. With both the head and the end cap installed, it is possible to pressure test the canister by covering one of the loop hose fittings with your hand and blowing into the other. No air should escape. If you hear or feel air leaking, remove the head and lid and confirm that all seals and O-rings are installed and properly cleaned and lubricated.

Installing the Scrubber Assembly

With the ExtendAir cartridge installed or the scrubber packed, the next step is to install the canister onto the bottom of the counterlungs. It should be oriented with the electronics head on the diver's left and the endcap on the diver's right (See **Figure 19**).



Figure 149 – Installing the Scrubber Assembly

With the canister in place, confirm that the fitting O-rings are present, clean, and lightly lubricated. Press the fittings into place, and then tighten the threaded rings. (See **Figure 20**).



Figure 20 - Scrubber Canister Installed



Mounting the Electronics/Battery Canisters

The electronics/battery canisters are mounted in elastic sleeves located on the bottom side of the outerbag in between the counterlungs and the scrubber canister. Carefully route the cables so that they are not pinched or kinked, and then insert the canisters into the elastic sleeves (See **Figure 21**).



Figure 21 – Electronics Canister Elastic Sleeves

With the canisters installed, connect the HUD and controller to their respective canister cables. The cables are color coded. Align and push the connectors together, then tighten the screw-together strain reliefs. The excess cable can now be tucked into the pouches on the inside of the counterlung outerbags (See **Figures 22 & 23**).



Figure 22 – Stowing Excess Cable



Figure 23 – Cables Stowed

Installing the Loop Hoses

There are two hoses that connect the DSV to the counterlungs to complete the breathing loop. Each hose has counterlung fittings attached to the end.



Before installing the hoses, lightly lubricate the O-rings and sealing surfaces on the counterlung fittings with Tribolube 71.

Install the loop hoses by pressing them into place and tightening the threaded rings. (See **Figure 24**).



Figure 24 - Installing Loop Hoses

Installing the DSV

Prior to installing the DSV it is recommended to visually inspect the mushroom valves on both sides of the unit. Ensure that there is no debris or excess lubrication on the sealing surface underneath the mushrooms. The mushrooms should be soft and pliable and sit flat against the valve cage. If the mushrooms do not sit flat or appear swollen, brittle, or damaged in any way, they must be replaced before diving. Faulty mushroom valves can cause hypercapnia, leading to severe injury or death.

Confirm that the mushrooms are sealing correctly by covering the exhale (right) side of the DSV with your hand and exhaling gently into the mouthpiece. There should be no air leaks heard or felt. Next, cover the inhale (left) side of the DSV and inhale gently. Again, there should be no leaks.

Once you have confirmed proper mushroom valve function, ensure that the O-rings and O-ring sealing surfaces are clean and lightly lubricated (See **Figure 25**) and then install the DSV.



Figure 25 - Lubricate DSV Sealing Surfaces



It should be oriented with the white locking buttons at the bottom with the DSV in the diver's mouth. The lever should also point down when the DSV is closed. Orientation of the DSV is critical as it determines the gas flow direction through the loop. The O2ptima CM will not function correctly if the DSV is reversed.

To install the DSV, connect the exhalation loop hose into the exhale side of the DSV by pushing the connector firmly into place. You may need to twist the lock ring slightly to align the tabs on the ring with the grooves in the DSV body. With the hose connector fully seated, push and turn the lock ring clockwise 1/8 of a turn until the white locking button snaps into the notch on the lock ring. Ensure that the lock ring is locked and that the hose cannot be pulled back out. Repeat the procedure to connect the inhalation hose to the inhale side of the DSV.



Figure 26 - Loop Hoses Installed

Installing the Oxygen Cylinder, Regulator and Hoses

Install the first stage onto the cylinder oriented as shown in figure 27.



Figure 27 - Oxygen Cylinder Installed



Clip the scrubber canister cover clips together and tighten the straps to snug the cover around the scrubber. The cylinder can now be mounted to the SMP attached to the bottom of the cover using the two cam straps. Orient the cylinder with the first stage to the diver's right and facing up as shown in **Figure 28**.



Figure 28 – First Stage Installed

Route the green hose of the hose assembly through the daisy chain and thread it onto the solenoid fitting (See **Figure 29**). This connection only needs to be hand tight.



Figure 29 – Oxygen Solenoid Connection

Route the black BC hose through the daisy chain and connect it to the oxygen MAV. Then thread the hose from the first stage through the daisy chain and connect it to the “Y” block as shown in **Figure 28**. Ensure that the second black hose is plugged into the Oxygen Manual Add Valve (MAV).



Figure 28 – Oxygen Hose Routing



Basic Operation & Use



WARNING: This manual does NOT cover all information and procedures required to safely dive the O2ptima CM and is NOT a substitute for unit specific training.

Harness Attachment

The O2ptima CM attaches using two bolt snaps on the shoulders and two bolt snaps on the waist. It may be worn with any harness system that can allow a high shoulder mounted D-ring on the top of each shoulder, as well as a D-ring on each hip on the waist belt. Dive Rite recommends the Nomad LS sidemount harness, however the O2ptima CM can be used with a backplate and wing or even single tank BC's as long as it can accommodate the proper D-ring placement.

For proper work of breathing, the O2ptima CM should be attached as high as possible on the chest. The counterlungs should sit just below the chin. Adjust the length of the straps holding the bolt snaps for a snug fit against the waist.

Oxygen Sensor Calibration

Oxygen sensor calibration should be confirmed prior to every dive and recalibrated as needed. Begin by disconnecting the counterlungs from the scrubber canister. Next insert the supplied calibration caps by pressing them into the fittings on the electronics head and end cap. The cap with the mushroom exhaust valve should be inserted into the electronics head fitting, and the cap with the BC fitting inserted into the end cap fitting.

With the oxygen cylinder valve turned off, disconnect the oxygen hose from the "Y" block and connect it to the calibration cap.

Turn on the Petrel 2 controller and HUD.

While watching the PPO2 values on the controller and HUD, turn on the oxygen cylinder valve in short bursts a couple of seconds apart. The PPO2 values on all sensors should climb as oxygen is added. Continue adding oxygen until all sensor values stabilize and do not continue to increase.

Once all values have stabilized at their maximum value, perform the calibration. See the **Shearwater Petrel Dive CAN Rebreather Controller Model Operations Manual** and the **Shearwater HUD User Manual** respectively for specific calibration instructions.

It is recommended to calibrate using 100% O2 if available, however it is possible to calibrate the controller using as low as 70% O2 if that is all that is available. If using a calibration gas less than 100%



O₂, the calibration FO₂ setting will need to be adjusted in the controller first. See the **Shearwater Petrel Dive CAN Rebreather Controller Model Operations Manual** for more information on this.

DSV Operation

The purpose of the DSV (Dive/Surface Valve) is to produce a one way flow of gas through the breathing loop. This is accomplished through the use of two one-way mushroom valves. When the diver inhales, the exhale valve closes and the inhale valve opens. When the diver exhales, the inhale valve closes and the exhale valve opens. It is extremely important that the integrity of the mushroom valves be maintained. These can quickly and easily be inspected between dives.

Any time the diver is not actively breathing on the loop, the DSV should be closed by pulling down on the lever arm until it is rotated to point straight down. It is important to close the valve before removing the mouthpiece from your mouth while underwater, or on the surface, to prevent water from entering the breathing loop and flooding the unit. Minor amounts of water in the loop can be dealt with by flushing it out of the exhalation counterlung OPV (this is a skill you will learn in class), however a major flood will not be recoverable during the dive and will require bailing out to an independent open circuit system.

If you are switching back to the DSV from a different breathing source while underwater, you will need to clear the small amount of water in your mouth and the mouthpiece before opening the DSV. Do this by exhaling through the DSV mouthpiece for several seconds before opening the lever. There is a small purge hole in the bottom of the DSV that allows removal of this water before opening (See **Figure 29**).



Figure 29 - DSV Water Purge Hole

You will hear or feel air bubbles escaping once the water is cleared. Then you can open the DSV by rotating the lever until it is fully opened and pointing straight forward.

Breathing on the Loop

The number #1 rule for diving a rebreather is to **ALWAYS KNOW YOUR PPO₂**! This can be monitored using the HUD and/or the controller. It is important to check both often and confirm that the PPO₂ values agree. If you cannot read the PPO₂ values or if for any reason you are unsure of the true PPO₂ in the loop you must bail out to an independent, open circuit bailout system.



It is important to remember that YOU are the engine that drives the breathing gas through the loop. You are using your lungs to push and pull gas through the unit. Proper functioning depends on this constant flow of gas. Breathing should be slow, deep, and continuous with no pauses. Pausing between breaths can cause PPO2 spikes because injected O2 does not flow across the sensors without the gas being “pushed” across them. If the injected O2 does not reach the sensors quickly enough, the controller will continue to add more O2 to try to maintain the setpoint. This can cause more O2 than necessary to be injected and lead to a spike once breathing is resumed and all of the injected oxygen hits the sensors at once.

It is also important to exhale completely to prevent CO2 buildup in your body. Shallow breathing does a poor job of expelling CO2 and can lead to hypercapnia. Breathing too fast can also be problematic as this does not allow proper dwell time of the exhaled gas in the scrubber (commonly referred to as “over breathing” the scrubber). Strive for a slow, steady breathing rhythm.

It is best to maintain a minimal loop volume when diving. This is achieved when a full inhalation does not quite trigger the ADV. Too much gas in the loop can have a negative effect on breathing effort and buoyancy control.

Electronic vs Manual Operation

The O2ptima CM is a fully electronics controlled rebreather (eCCR), but it is also capable of manual operation (mCCR). When using the O2ptima CM in eCCR mode, the controller is analyzing the oxygen sensor values in real time and determining when and how long to fire the oxygen injection solenoid in order to maintain the user adjustable PPO2 setpoint. When all systems are functioning properly, the diver will not have to manually add any gas to maintain a breathable loop.

It is important to keep in mind that the rebreather is only a machine. The controller is taking readings from the oxygen sensors, and making determinations based on those readings. If the values that the sensors are providing are not accurate, then the end result will not be accurate either. There are a variety of reasons that the oxygen sensor values may not accurately reflect the actual PPO2 of the gas in the breathing loop. Some of these reasons can be aging, damaged, or current limited sensors, wiring harness or electronics issues, water or other contamination on the face of the sensors, and improper breathing of the diver.

Because of this, it is up to the diver to monitor the HUD and controller, interpret the information provided, and take action if necessary. All of these issues and the correct responses to take will be covered by your instructor during class. The most important things to keep in mind are that the rebreather cannot think for you, and “when in doubt, bail out!”

The O2ptima CM can also be used manually. In this case the diver monitors the PPO2 readings on the HUD and controller, and manually injects oxygen into the breathing loop by pressing the manual addition valve on the exhalation counterlung. This gives the diver complete control over the PPO2 in the loop. There are several scenarios in which the diver might choose to use manual control such as a solenoid failure or partial electronics failure.

It is also possible to keep the O2ptima CM in eCCR mode, but lower the PPO2 setpoint, and then manually inject oxygen to maintain a higher setpoint. In this way the user is operating the unit manually with the electronics functioning as a sort of “parachute” in case the diver becomes distracted or is unable to manually add oxygen.



All of these scenarios and operation modes will be covered in your training class.

Dive Rite recommends diving the O2ptima CM with a PPO2 setpoint of between 0.7 and 1.2 depending on the dive. Diving at PPO2s higher than 1.2 can increase the risks of oxygen toxicity.

Diluent Injection

Diluent is injected into the breathing loop in one of two ways—either automatically through the ADV/MAV, or manually by pressing directly on the ADV/MAV diaphragm.

The ADV is a demand valve and functions similarly to a standard 2nd stage. If the counterlungs fully collapse when the diver inhales, the negative pressure on the ADV diaphragm will cause the valve to open and add diluent. This allows the diver to take a full breath even if the counterlungs are “bottomed out.” This can be especially useful on descent where the loop volume is decreasing due to increasing water pressure.

Manually injecting diluent is also an option and may be used to perform a diluent flush. These skills will be covered in your class.

Servicing, Maintenance, & Cleaning

In order for the O2ptima CM to continue to perform properly, it must be cleaned and maintained regularly. Rebreathers require more maintenance and cleaning than standard open circuit SCUBA equipment. For their own safety, a rebreather diver should be committed to spending the time, effort, and money required to properly maintain the unit.

Post Dive Procedures and Cleaning

There are several things that should be done as soon as possible after the dive is over.

First, close the DSV and change your set point to 0.19 PPO2 on the controller. This will prevent the unit from firing the solenoid and wasting oxygen when the unit is not in use.

Next, it is good to check the battery voltages to know if the batteries will need replacing before the next dive.

Also, note the pressure remaining in the oxygen and diluent cylinders, and the total dive time to determine scrubber usage.

The cylinder valves can now be closed and the lines purged by pressing the manual add buttons.

(Never turn off the cylinder valves before you are out of the water and have removed the rebreather! **)**

If the unit was dived in salt water, soak it in a freshwater tank if possible and then spray it off thoroughly with fresh water.

Turn off the controller and HUD to maintain battery life. Make sure the electronics do not come back on automatically due to the wet switch.



This is all that is needed if the unit will be dived again that day. Otherwise, the breathing loop should be disassembled and sterilized. It is recommended to do this within 12 hours after diving to prevent the growth of mold and bacteria in the loop.

Begin the cleaning procedure by disassembling the loop. Remove the DSV, loop hoses, counterlungs, scrubber end cap, and scrubber canister.

It is not necessary to remove the electronics head from the unit for cleaning. Simply wipe down the inside of the head with a clean towel and allow it to dry.

Remove the EAC scrubber cartridge or granular media and discard. All of the other pieces of the loop can now be thoroughly flushed under warm running water paying special attention to the inside of the exhalation side hose and counterlung.

Next, mix up a solution of Steramine in a bucket according to the directions on the bottle. Submerge all loop parts except for the electronics head and the counterlungs in the solution for a minimum of 1 minute to sterilize. Do not leave them in the solution for an extended period of time, as over exposure to the chemicals can damage mushroom valves and seals.

Once sterilized, remove the parts from the solution and thoroughly rinse inside and out with fresh warm water.

To sterilize the counterlungs use a cup to pour some of the Steramine solution into each counterlung. Cover the openings and shake the counterlung for 1 minute, then dump and rinse the inside thoroughly with fresh warm water.

Shake excess water off of all the components and then spread them out on a clean towel to dry. Hang the loop hoses and counterlungs to dry. Allowing components to dry completely is the best defense against the growth of mold and bacteria.

For reference, see the Post Dive Checklist in the **Checklists** section.

Oxygen Sensor Care

Oxygen sensors are the Achilles' heel of all modern rebreathers. Sensors have a finite life span and should be considered consumable items. They are prone to failure and it is important to know how and why they can fail.

Oxygen sensors are essentially oxygen powered galvanic fuel cells. They are electrochemical devices that produce a weak electric current in the presence of oxygen. Over time, the chemicals are slowly consumed and the sensor becomes increasingly unreliable.

A new sensor will have a linear response to the partial pressure of oxygen throughout the normal operating range used in rebreather diving. However, as they age, their output becomes increasingly non-linear at higher partial pressures of oxygen. This is commonly referred to as "current limiting." The problem with this is that a sensor may appear to be acting normally, but display a lower PPO₂ than what is actually in the breathing loop. If the diver (or electronic controller) is using this value to determine oxygen injection it can quickly lead to a hyperoxic breathing loop.

This is the primary reason for having multiple oxygen sensors. It allows the diver (or controller) to look at all sensor values simultaneously and easily determine if one is giving a different reading from the rest. If a discrepancy occurs, the diver has several options available to determine which sensors are reading



correctly and which should be ignored. These procedures will be covered in your training. Any sensors that are suspected of being current limited must be replaced before diving the unit.

The response time of aging sensors will also slowly increase. If you notice one or more sensors responding slowly to changes in PPO2 compared to the other sensors, they should be replaced.

Many rebreather fatalities have occurred because of using old sensors. Dive Rite recommends that sensors be used for no more than 12 months. The clock starts ticking as soon as the sensor is removed from the original packaging. The 12 month limit is independent of the number of dives on the unit. Even if the rebreather is stored and unused for a long period of time, the sensors should still be replaced prior to diving if they have been installed for more than 12 months.

Even unused sensors still in their original packaging have a limited shelf life. Dive Rite uses Analytical Industries, Inc. and American Sensor Technologies, Inc. sensors which both have a “Sell by” date of 4 months after manufacture and a “Do not use after” date of 16 months after manufacture. Even if the sensor has been in use for less than 12 months and seems to be working correctly, it should be discarded and replaced once the “Do not use after” date is reached.

Because of the limited shelf life, it is recommended that you do not keep a large stock of “backup” sensors. It is much better to purchase fresh sensors as they are needed.

There are different theories about the best replacement schedule for sensors. Many divers opt to replace all four sensors at once during the annual service every year.

An alternative replacement schedule is to replace one sensor every 3 months. The sensor that is replaced should either be the oldest of the set, or alternatively the one that is the slowest to respond to PPO2 changes. This method has the advantage that each sensor will be from a different manufacturing batch. Although rare, it is possible for an entire batch of sensors to be defective and fail prematurely. The age of the sensors will also be staggered with this method and will lessen the chance that multiple sensors will fail at the same time.

Replacing sensors in a timely manner will mitigate a lot of the potential issues, however it is possible for sensors to fail before their expiration date is reached. Even brand new sensors can fail. It is always best to keep a close eye on your HUD and controller for any discrepancies and replace any suspect sensors immediately.

Sensors should not be removed from the unit for storage in between dives. This practice is unnecessary and can lead to damaged sensors and increased wear and tear on the wiring harness.

Sensors should never be frozen, vacuum sealed, or stored in inert gas or desiccant in an attempt to increase their life span. Any of these practices will likely damage the sensor. Sensors, along with the rest of the rebreather, are best stored in a cool (but not freezing), dry location out of direct sunlight.

For more information on oxygen sensors see Appendix II: **Galvanic Oxygen Sensors Applied to Closed Circuit Rebreathers** by Analytical Industries, Inc. and Analytical Industries, Inc. (www.aii1.com)



Oxygen Sensor Replacement

To replace a sensor, remove the screw holding the sensor plate in place (See **Figure 30**).

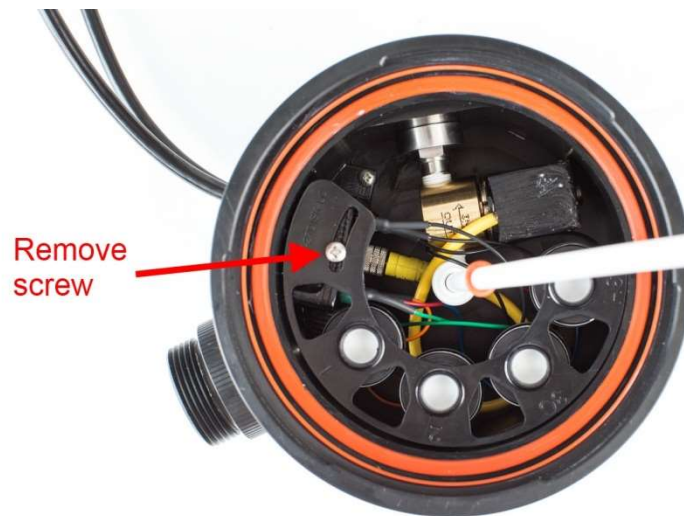


Figure 30 - Sensor Plate Screw

Lift the sensor plate and carefully unplug the sensor to be replaced at the back of the sensor. Lift the connector tab to remove—do not pull on the wires (See **Figure 31**).

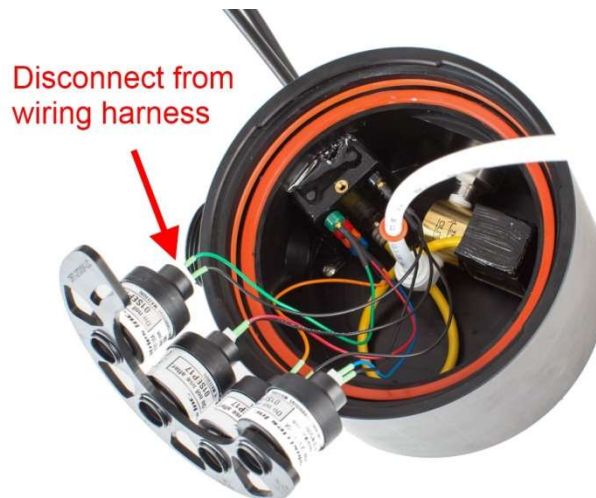


Figure 31 – Oxygen Sensor Wiring Harness

The sensors are threaded into the sensor plate. Remove the sensor by turning it counterclockwise (See **Figure 32**).



Figure 32 - Sensor Removal

Install the new sensor by threading it into the plate. Finger tight is fine; do not over tighten. The front edge of the sensor should protrude slightly past the surface of the sensor plate (See **Figure 33**). This is intentional and encourages any water condensation on the sensor plate to drip off instead of easily running into the sensors.

Plug the wiring harness into the sensor verifying the sensor position number on the sensor plate corresponds to the correct wire at the connector block.

Finally, reinstall the sensor plate with the sensor plate screw.

Once the sensor is installed, perform an oxygen flush and calibration (See the **Oxygen Sensor Calibration** section). Verify that the sensor is reading correctly before diving.



Figure 33 - Sensors Installed



Battery Replacement

There are 3 batteries on the O2ptima CM. The first is the internal battery located inside the controller. The controller displays this battery voltage in yellow when the battery is low and needs replacement. It will display flashing red when the battery is critically low and must be replaced as soon as possible. To replace this battery, see the **Changing the Battery** section of the **Shearwater Petrel Dive CAN Rebreather Controller Model Operations Manual**.

The other two batteries are located inside the external electronics/battery canisters. One canister houses the battery that powers the SOLO board as well as the solenoid. This battery is a standard 9 volt battery.

The external battery voltage for the SOLO/solenoid battery can also be checked on the controller. This voltage is only checked when the solenoid is fired, so if the solenoid has not yet fired the value is unknown and displays as a yellow “?”. If this is the case, adjust the controller setpoint to a higher PO2 and allow the solenoid to fire for several seconds and then recheck the voltage.

The second canister contains the battery which powers the OBOE board and HUD. This battery is a standard AA type. The HUD does not have its own battery—it only receives power from the OBOE board.

A low OBOE/HUD battery voltage will be displayed on the HUD. After turn on, the yellow row of LEDs will remain on for 30 seconds to indicate a low battery that should be replaced.

A high quality alkaline 9V battery will typically provide approximately 50-60 hours of dive time before needing replacement. However, there is a slight battery drain at all times when the batteries are in place even if the HUD and controller are turned off. If the unit is stored for an extended period of time with the batteries in place, the batteries may need replacing even if the unit has not been used.

Typically, the SOLO/solenoid 9V battery will need changing more frequently than the OBOE/HUD AA battery. Dive Rite recommends changing both batteries at the same time once either one indicates a low battery voltage. Rechargeable batteries are not recommended for use in these locations. Only high quality, name brand batteries are recommended. It is important to remember that this is **LIFE SUPPORT** equipment—this is not the place to be cheap on batteries. For the correct replacement batteries, please see the **Battery Recommendations** section below.

To replace either of the external canister batteries, begin by unscrewing the cap on the end of the canister. While unscrewing the cap, hold the canister with the cap pointed down. This will prevent any residual water that might be located on the sealing O-rings or cap threads from running down into the canister and damaging the electronics (see **Figure 34**). With the cap removed, carefully dry any excess water before proceeding.

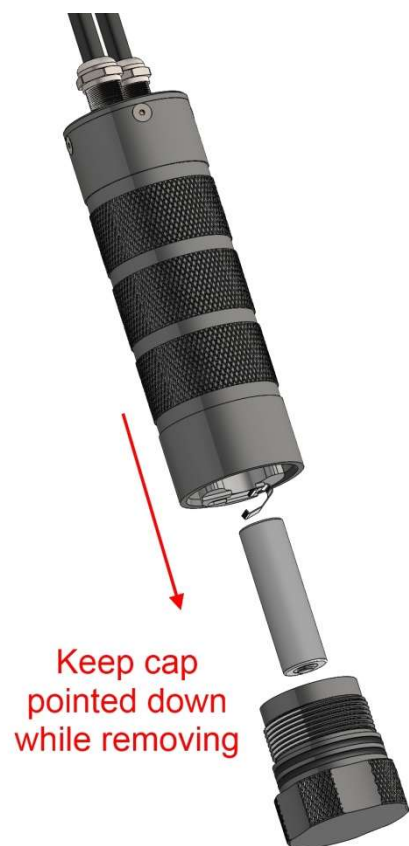


Figure 34 - Cap Removal & Battery Replacement



The battery can now be replaced paying special attention to the “+” and “-” orientation as marked on the canister.

Inspect the canister O-rings before reinstalling the cap. They should be clean and undamaged. If needed, carefully remove the O-rings and wipe them clean along with the O-ring grooves on the cap. Lightly lubricate the O-rings with a silicone grease such as Dow Corning Molykote 111.

With the O-rings correctly in place, reinstall the canister cap by threading it into the body. The cap only needs to be hand tight. Do not over tighten.

Battery Recommendations

Battery Location	Battery Type	Recommended Batteries	Acceptable Alternatives
Petrel 2 Controller (Internal)	AA	<ul style="list-style-type: none"> Duracell Coppertop or equivalent high quality AA 1.5V Alkaline 	<ul style="list-style-type: none"> Saft 3.6V LS14500 3.7V Li-Ion 14500 rechargeable (AW brand is preferred) 1.2V Ni-MH rechargeable Photo Lithium 1.5V (recommended for cold water use) Low cost Zinc-Carbon 1.5V batteries will work, but are not recommended due to poor performance and short life
SOLO/Solenoid External Canister	9V	<ul style="list-style-type: none"> Ultralife 9V Lithium¹ 	<ul style="list-style-type: none"> Duracell Coppertop or equivalent high quality 9V Alkaline¹ <p>*** Rechargeable batteries are NOT recommended***</p>
OBOE/HUD External Canister	AA	<ul style="list-style-type: none"> Energizer Ultimate Lithium AA 	<ul style="list-style-type: none"> Saft 3.6V LS14500 Duracell Coppertop or equivalent high quality AA 1.5V Alkaline <p>***Rechargeable batteries are NOT recommended***</p>

¹Note: Not all 9V batteries are the same size. Some brands will not fit correctly into the battery canister. Confirm that the battery fits loosely into the cap before inserting the battery and tightening the cap. Failure to do this can lead to damage of internal components.

Storage

If you plan to store your O2ptima CM without use for an extended period of time there are several steps you should take to protect the unit.

First, remove all batteries from the unit. This includes the AA battery in the Petrel 2 controller, the 9V battery in the SOLO/solenoid external canister, and the AA battery in the OBOE/HUD external canister. There is a slight current draw on the batteries even when the unit is turned off. Also, alkaline batteries tend to leak when they are fully discharged.



You will want to perform a thorough cleaning and sterilization of the entire breathing loop and then allow it to dry completely in pieces before storage.

Store all pieces in a sealed box and/or a plastic bag to keep bugs from getting inside of the components. The unit should be stored in a cool, dry environment away from direct sunlight.

It is not recommended to remove the oxygen sensors for storage. However, all sensor dates should be inspected after a long period of storage to ensure that they have not expired. Replace any expired sensors, install fresh batteries, and perform a sensor calibration before diving the unit.

Annual Service

Once every year you should return your O2ptima CM to Dive Rite or an approved Dive Rite O2ptima service center for an annual service. This service includes replacement of O-rings, loop hoses, and oxygen sensors, along with a rebuild of the DSV and regulators, and checks of the electronics to confirm correct operation and up to date firmware. This is not a user permitted service. It must be performed by an authorized service center.

Recommended Care Products

Use	Description
Dive Rite DSV Lubrication	Aerospace Lubricants Tribolube 71
LP and HP Hose O-ring Lubrication	Aerospace Lubricants Tribolube 71
Loop Hose O-ring Lubrication	Aerospace Lubricants Tribolube 71 or Dow Corning Molykote 111
HUD & Controller Connector Lubrication	Dow Corning Molykote 111
Electronics/Battery Canister Lid O-ring Lubrication	Dow Corning Molykote 111
Breathing Loop Disinfectant	Steramine Sanitizing Tablets diluted in fresh tap water according to the packaging directions
General Cleaning (rinsing saltwater, etc.)	Fresh tap water

Technical Specifications

Weight	14 lbs 6 oz (6.5 kg) without cylinders or scrubber media
Oxygen Cylinder	Aluminum 13cf (2L) Cylinder (recommended)
Oxygen 1 st Stage Intermediate Pressure	85 psi
Diluent 1 st Stage Intermediate Pressure	140 psi
Batteries	Petrel 2 Controller (Internal): AA



	SOLO/Solenoid External Canister: 9V OBOE/HUD External Canister: AA
Counterlung Volume	6 Liter Total Loop Volume
Maximum Operational Depth	Max Depth 40 m (130 fsw) with Air diluent Max Depth 100 m (330 fsw) with Trimix diluent *Dives exceeding 100 m (330 fsw) are associated with numerous additional risks
Operating Temperatures	+39°F to +90°F (+4°C to +32°C)
Short-Term (hours) Temperature Range	-4°F to +122°F (-20°C to +50°C)
Long-Term Storage Temperature Range	+41°F to +68°F (+5°C to +20°C)
Oxygen Sensors	Analytical Industries, Inc. or American Sensor Technologies, Inc. type R22D sensors (X 4)
Oxygen Sensor Operational Voltages	8 – 14 mV in air @ sea level 40 – 65 mV in pure oxygen @ sea level
Oxygen PPO2 Setpoint Range	0.5 – 1.5 PPO2 during dive mode (0.19 PPO2 available in surface mode only)
Water Traps	2 water traps—one located inside the scrubber lid and one inside the exhaust counterlung bladder
Electronics	Shearwater DiveCAN Petrel 2 Controller Shearwater DiveCAN HUD (Shearwater NERD optional)
Scrubber Media	Micropore ExtendAir Cartridges (EACs) or granular scrubber media: Intersorb 812 or Sofnolime 797 (8-12 mesh)
Granular Scrubber Capacity	Approximately 5 lbs (2.2 kg) (will vary slightly depending upon granular type and packing method)



Revisions & Changes in Documentation

Revision	Date	Description
Rev A	3/23/20	Original document
Rev B	4/22/20	Typo corrections, bolded important notes, updated water trap tubes
Rev C	10/6/20	Added scrubber filter and AST sensor information

Checklists

Checklists are provided on the following pages. Note that there is a “Assembly Guide Checklist” and also a “Survival Checklist.” These are redundant. The “Assembly Guide Checklist” is intended as a complete assembly checklist to be used by students in training, or anyone who has not used the rebreather for a period of time and would like a detailed assembly checklist to follow. Some divers will choose to use this list exclusively and print out multiple copies to use as their dive log.

The “Survival Checklist” is intended for users who are thoroughly familiar with assembling and operating the O2ptima CM and are actively using it. It provides a condensed list of the critical checks that must be performed before every dive. If multiple dives are performed in a single day, this list should be used before every dive.

The “Preflight Checklist” is intended to be performed after gearing up and just before entering the water to begin your dive. It will confirm that all systems are turned on and functioning properly. It is recommended to attach a copy of this checklist to the O2ptima in a convenient location.

The “Post Dive Checklist” should be used after the dive is over. There are two sections to this list. The first is things that should be done immediately after every dive after getting out of the water, and the second is things that should be performed at the end of your day of diving.